

University of California

Ernest O. Lawrence  
Radiation Laboratory

PARTICLE-BEAM-PROFILING-SYSTEM

TWO-WEEK LOAN COPY

This is a Library Circulating Copy  
which may be borrowed for two weeks.  
For a personal retention copy, call  
Tech. Info. Division, Ext. 5545

Berkeley, California

## DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

Submitted as a Note to  
Review of Scientific Instruments

UCRL-17213  
Preprint

UNIVERSITY OF CALIFORNIA

Lawrence Radiation Laboratory  
Berkeley, California

AEC Contract No. W-7405-eng-48

PARTICLE-BEAM PROFILING SYSTEM

Robert E. Gilmer, Franklin D. Neu, Robert J. Sprafka,  
and Joseph E. Strople

October 18, 1966

PARTICLE-BEAM PROFILING SYSTEM\*

Robert E. Gilmer, Franklin D. Neu, Robert J. Sprafka,  
and Joseph E. Strople

Lawrence Radiation Laboratory  
University of California  
Berkeley, California

October 18, 1966

ABSTRACT

A system is described for oscilloscope display of a particle-beam profile, which was built for an experiment at the Stanford Linear Accelerator Center.

We have constructed a novel beam-profile system for use in a beam experiment at the Stanford Linear Accelerator Center (see Fig. 1). The system displays single-particle spark-chamber events on the face of a storage oscilloscope, accumulating the events to give a beam profile at the plane where the spark chamber is placed. This allows the experimenter to find easily the exact position and focus of his particle beam when setting up his experiment.

When a particle passes through the spark chamber, a trigger pulse fires the spark gap (Fig. 2), which puts a high-voltage, 200-nsec pulse on the spark chamber (Fig. 3).

The top conducting surface of the chamber has small copper wires in a parallel array 1 mm apart and connected to a common bus on only one end. The bottom conducting surface is similarly constructed (see Fig. 4), but its wires are oriented at 90 deg to those on the top surface. The two faces are ~1 cm apart. The particle-sensing area of the chamber is 25.4 cm square. Cloth made of wire in one axis and fiberglass thread in the other is used for the chamber faces. This cloth was glued with epoxy adhesive to laminated fiberglass sheets for backing, and the chamber faces were glued with epoxy cement to plastic spacers. The space between the faces is filled with neon gas. (See Figs. 4 and 5.)

When the chamber is pulsed, arcs occur in the neon along the ionized path left by the particle, and a large current of 25 to 50 A flows through one wire in the top face, or X axis, and through a wire in the bottom face, or Y axis. This current flows past an iron-cobalt metal strip in the X and Y axis, as it flows from the top face common bus to

the bottom face common bus.<sup>1</sup> The iron-cobalt wires, which are electrically insulated from the chamber-face wires, connect to magnetostrictive sensors. The current pulse in the chamber-face wires creates a sonic pulse in the iron-cobalt wire where the current passes under the magnetostrictive wire. This sonic pulse is detected by a magnetostrictive sensor, as are the fiducial sonic pulses.

Reference wires are run under the iron-cobalt wire near the first and last copper chamber wire. These wires are pulsed with current when the chamber is pulsed, and are used for fiducials to start the coordinate and fiducial scalars, and to stop the fiducial scalars.

The X and Y coordinate and fiducial counters start counting at a 10-MHz rate when the magnetostrictive sensor and pulse center-finder circuit detect the first X and Y fiducial sonic pulses, respectively; the X and Y coordinate counters stop on the second X and Y pulses, respectively; the X and Y fiducial counters stop on the third pulses, respectively.<sup>2</sup> If the fiducial counters are not at the right count after the third detected pulse, the logic prevents display of the X- and Y-axis coordinates. More than one spark, or a chamber misfire, will cause the fiducial counters to have an incorrect value, because a second spark functions in the same way as the second fiducial pulse.

The X and Y counters feed a digital-to-analog-converter resistor ladder, and display lights. The X and Y digital-to-analog-converter outputs go to the X and Y storage-oscilloscope deflection amplifiers, respectively, and when the fiducial counts are correct after the spark chamber is fired, the oscilloscope intensity input is pulsed, storing the

spot on the oscilloscope face in direct relationship to the X and Y position of the particle path (see Fig. 5). The counter display lights are an aid to the operator.

The cables from the main control rack are long enough to allow the beam-profile spark chamber to be placed 15 meters from the control electronics.


FOOTNOTE AND REFERENCES

\* This work was done under the auspices of the U. S. Atomic Energy Commission.

1. Frederick A. Kirsten, Victor Perez-Mendez, and James M. Pfab, Development of Magnetostrictive Chamber Readouts, Lawrence Radiation Laboratory report UCID-2629, August 19, 1965.
2. Kai L. Lee and James M. Pfab, Magnetostrictive Pick-up Preamplifier, Lawrence Radiation Laboratory report UCID-2750, February 7, 1966.


FIGURE LEGENDS

- Fig. 1. Beam profile control electronic rack, with the spark chamber and magnetostrictive sensors shown on the top of a stand at the right, and the spark gap shown on the bottom shelf of the stand.
- Fig. 2. Spark gap and capacitor box for high-voltage-pulse distribution.
- Fig. 3. Spark chamber with magnetostrictive sensors.
- Fig. 4. Spark chamber and magnetostrictive sensor diagram.
- Fig. 5. Beam profile system block diagram.

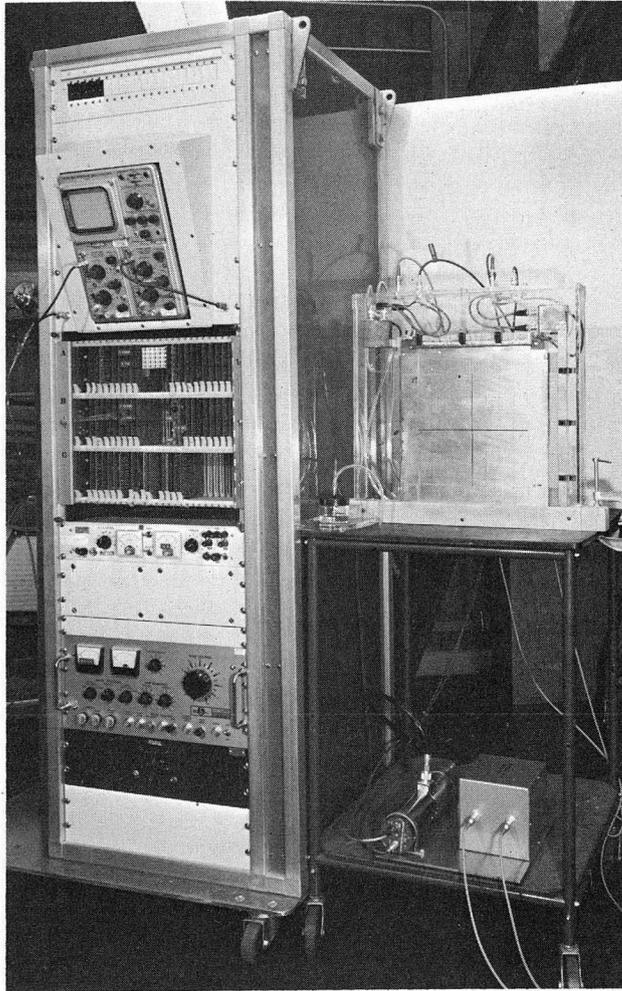


ZN-5988

Fig. 1

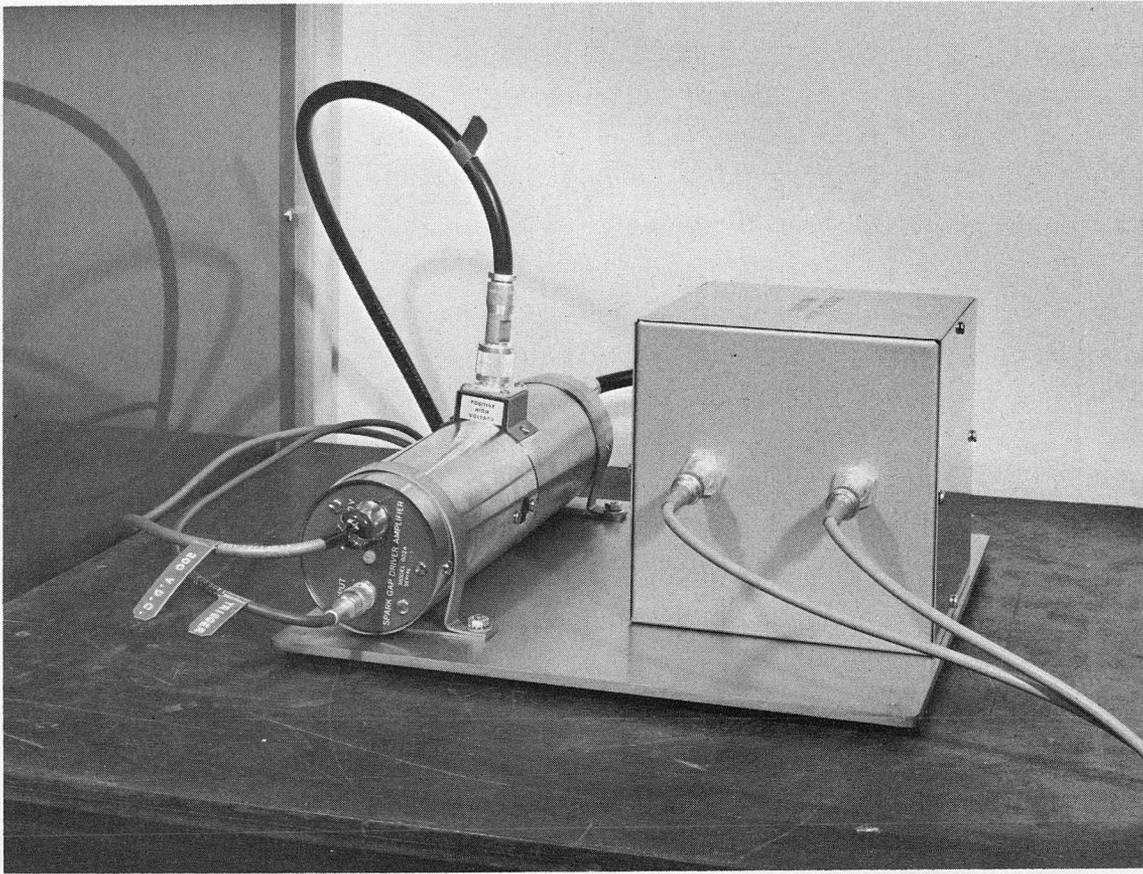


ZN-5986

Fig. 2

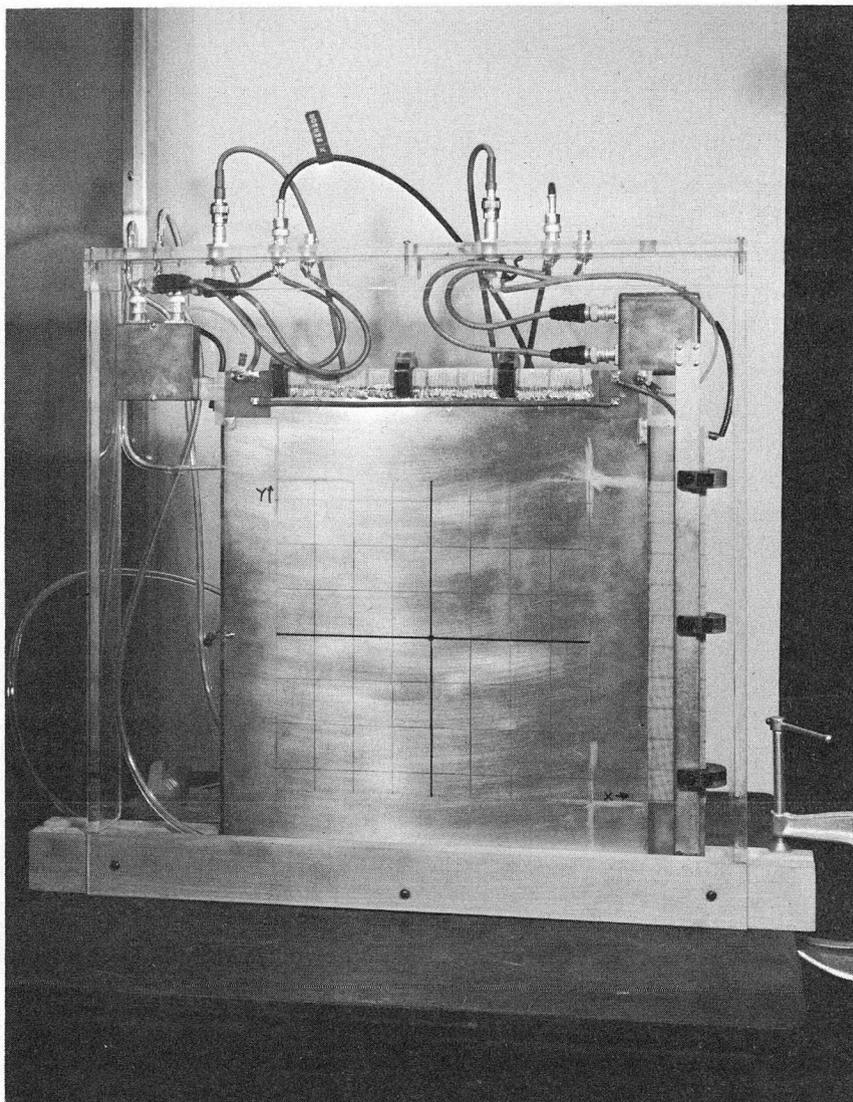


ZN-5987

Fig. 3

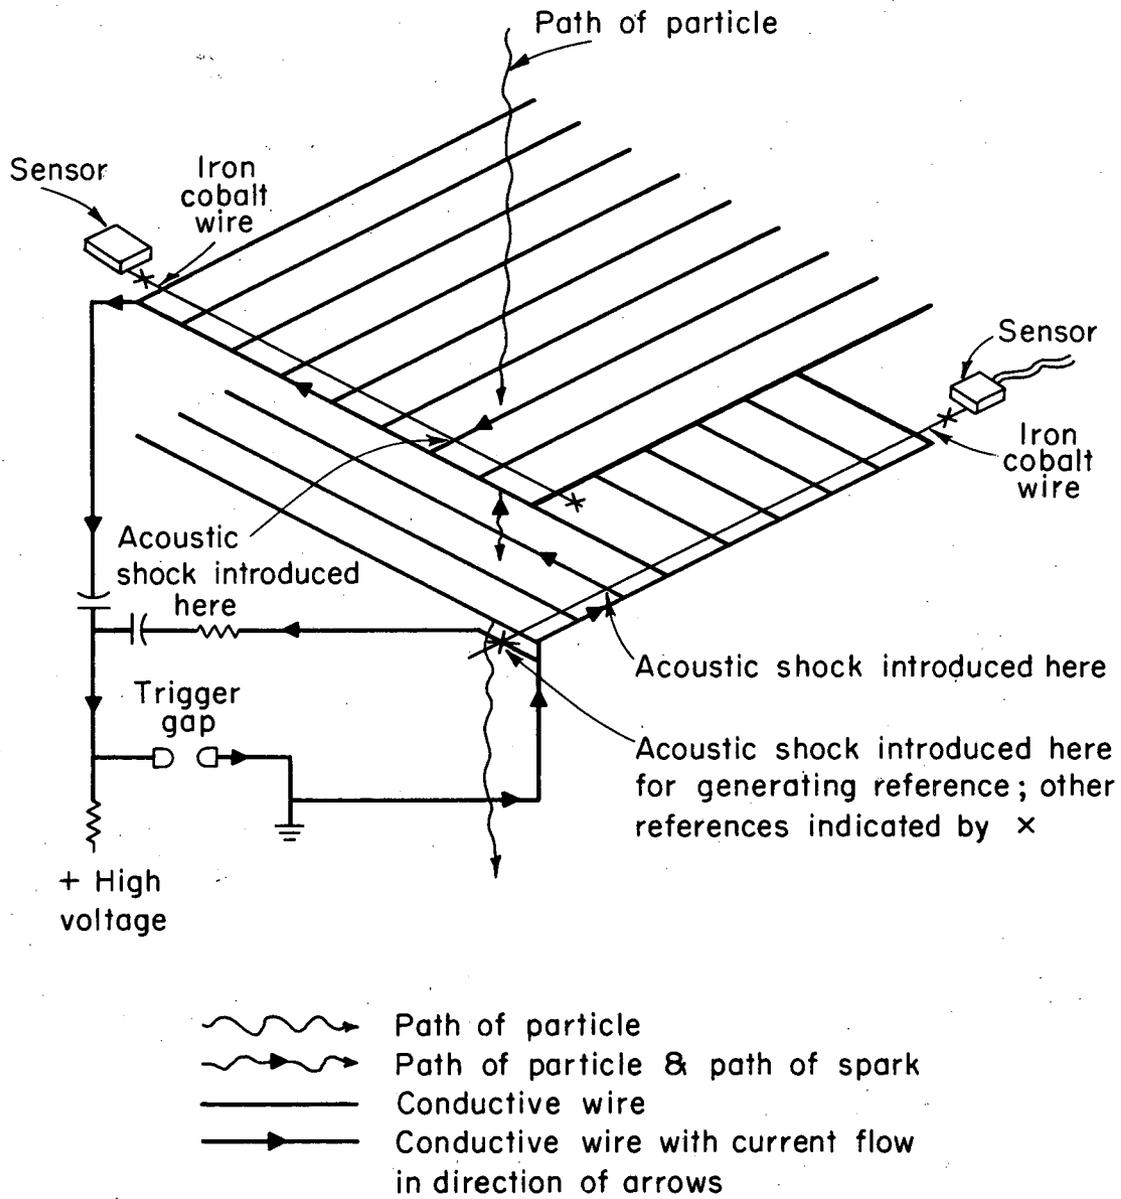

MUB-13625

Fig. 4

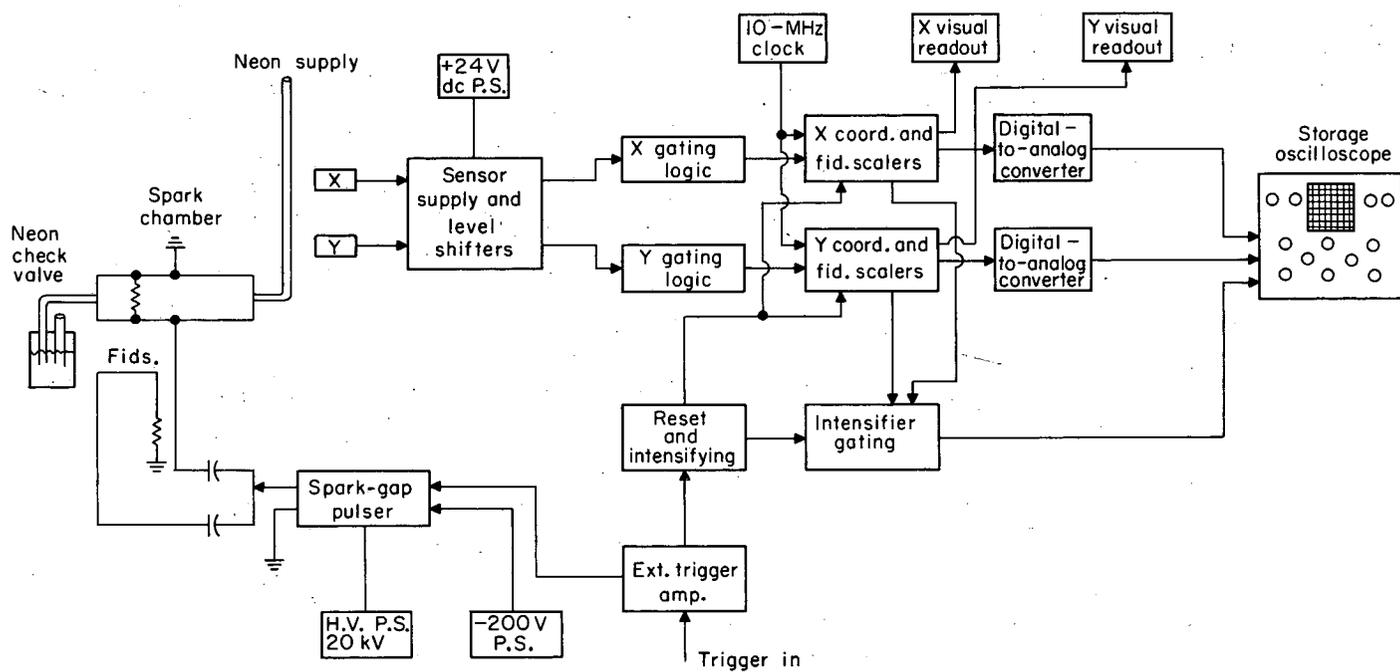

MU B-13626

Fig. 5

This report was prepared as an account of Government sponsored work. Neither the United States, nor the Commission, nor any person acting on behalf of the Commission:

- A. Makes any warranty or representation, expressed or implied, with respect to the accuracy, completeness, or usefulness of the information contained in this report, or that the use of any information, apparatus, method, or process disclosed in this report may not infringe privately owned rights; or
- B. Assumes any liabilities with respect to the use of, or for damages resulting from the use of any information, apparatus, method, or process disclosed in this report.

As used in the above, "person acting on behalf of the Commission" includes any employee or contractor of the Commission, or employee of such contractor, to the extent that such employee or contractor of the Commission, or employee of such contractor prepares, disseminates, or provides access to, any information pursuant to his employment or contract with the Commission, or his employment with such contractor.

