

UC-91
LBID-442



Lawrence Berkeley Laboratory


UNIVERSITY OF CALIFORNIA

ENERGY & ENVIRONMENT DIVISION

RECEIVED
LAWRENCE
BERKELEY LABORATORY

APR 28 1982

LIBRARY AND
DOCUMENTS SECTION

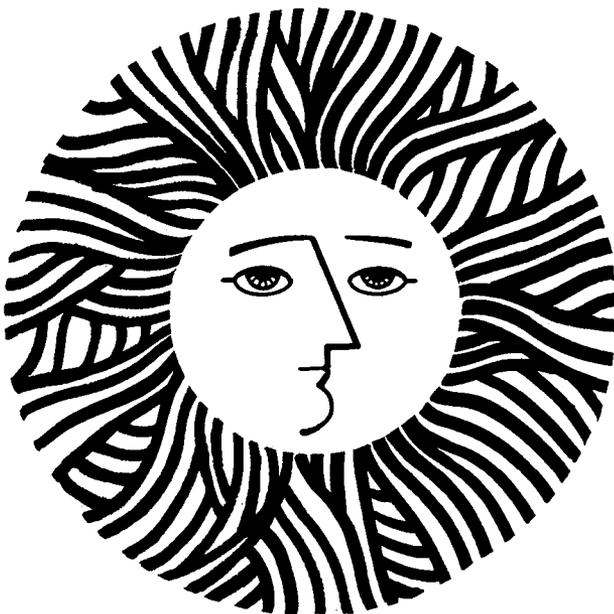

For Reference

Not to be taken from this room

LBID-442
e.1

DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

September 3, 1981

TO: Charles Grua

FROM: Richard H. Sakaji, Bonnie M. Jones, and Jerome F. Thomas;
Frank Pearson and Christian G. Daughton (SEEHRL)
Lawrence Berkeley Laboratory, University of California, Berkeley, CA 94720

RE: Monthly Progress Report for August
Steam Stripping Project
LBID- 442

ANALYTICAL METHODS DEVELOPMENT

Ammonia Determination

The following ammonia nitrogen values were obtained using Weatherburn's version of the phenate method: Oxy-6 gas condensate, 6759 ppm (rsd = 1.4%, n = 10); Oxy-6 retort water, 1089 ppm (rsd = 1.1%, n = 10); air stripped Oxy-6 gas condensate, 149 ppm (rsd = 1.3%, n = 9).

Samples of Oxy-6 gas condensate were spiked with 1000, 10 000, and 50 000 ppm ammonia nitrogen using a standard ammonium sulfate solution. Recoveries of ammonia nitrogen by Weatherburn's phenate method were 110%, 93%, and 100%, respectively. Our experimental results indicate that Weatherburn's version of the phenate method for ammonia determination may be applied to our wastewater samples.

Carbon Analysis

Samples of a known concentration of carbon (potassium acid phthalate) were analyzed using a Coulometrics carbon analyzer that was fitted with a Beckman ceramic combustion tube. A ceramic combustion tube, in comparison with a Coulometrics stock quartz combustion tube, is not attacked by the high salt concentration of synfuel wastewaters. The recoveries from two separate experiments were: 98 to 104% within the range of 1000 to 10,000 ppm carbon; 97 to 101% for 20 to 1000 ppm carbon; and 87% for 10 ppm carbon.

We also compared two methods of carbon determination, low-temperature UV-persulfate oxidation and IR detection (Dohrmann/Envirotech) vs. the high-temperature-combustion coulometric detection method of the Coulometrics carbon analyzer. Replicate samples of Oxy-6 retort water and gas condensate were analyzed by each method. Equivalent values for dissolved organic carbon, as well as for total carbon, were obtained by either instrument for a given

sample. This is the only form of validation that we have obtained for carbon determination of these waters.

STEAM STRIPPER DESIGN

Fabrication

The pressure vessels for steam generation, bottoms collection, and overheads capture were built and mounted on the support structure. To decrease heat loss and to minimize worker exposure to hot surfaces, some of the pressure vessels and pipework were insulated. The raw waste feed, condenser cooling water recycle, and flash evaporator recycle pumps were installed on the structural support. The installation of the steam and cooling water transfer lines was begun.

The control panel for the heaters, temperature read-out, pumps, and pressure read-out was installed and labelled. The wiring for the heater, digital temperature read-out, and other controls also was initiated.

LITERATURE REVIEW

Factors that affect the solubility of ammonia include pH, ionic strength, the presence of hydrogen sulfide, and the ratio of carbon dioxide to ammonia. For instance, in a solution of carbon dioxide and ammonia of constant normality, as the mole ratio of carbon dioxide to ammonia increases, the partial pressure of the ammonia over the water decreases. These factors must be taken into consideration in calculations used to construct equilibrium curves. We are conducting a literature review for data on ammonia solubility in solutions containing hydrogen sulfide and carbon dioxide. These data will enable us to model the equilibrium curves. From these curves, we will calculate both the number of transfer units and the height equivalent to a transfer unit that are required to achieve predetermined levels of removal.

This work was supported by the U.S. Department of Energy under Contract number DE-AC03-76SF00098.

This report was done with support from the Department of Energy. Any conclusions or opinions expressed in this report represent solely those of the author(s) and not necessarily those of The Regents of the University of California, the Lawrence Berkeley Laboratory or the Department of Energy.

Reference to a company or product name does not imply approval or recommendation of the product by the University of California or the U.S. Department of Energy to the exclusion of others that may be suitable.

TECHNICAL INFORMATION DEPARTMENT
LAWRENCE BERKELEY LABORATORY
UNIVERSITY OF CALIFORNIA
BERKELEY, CALIFORNIA 94720