LBID-511
c.1

Lawrence Berkeley Laboratory

UNIVERSITY OF CALIFORNIA

Engineering & Technical Services Division

RECEIVED
LAWRENCE
BERKELEY LABORATORY

MAY 24 1982

LIBRARY AND
DOCUMENTS SECTION

For Reference

Not to be taken from this room

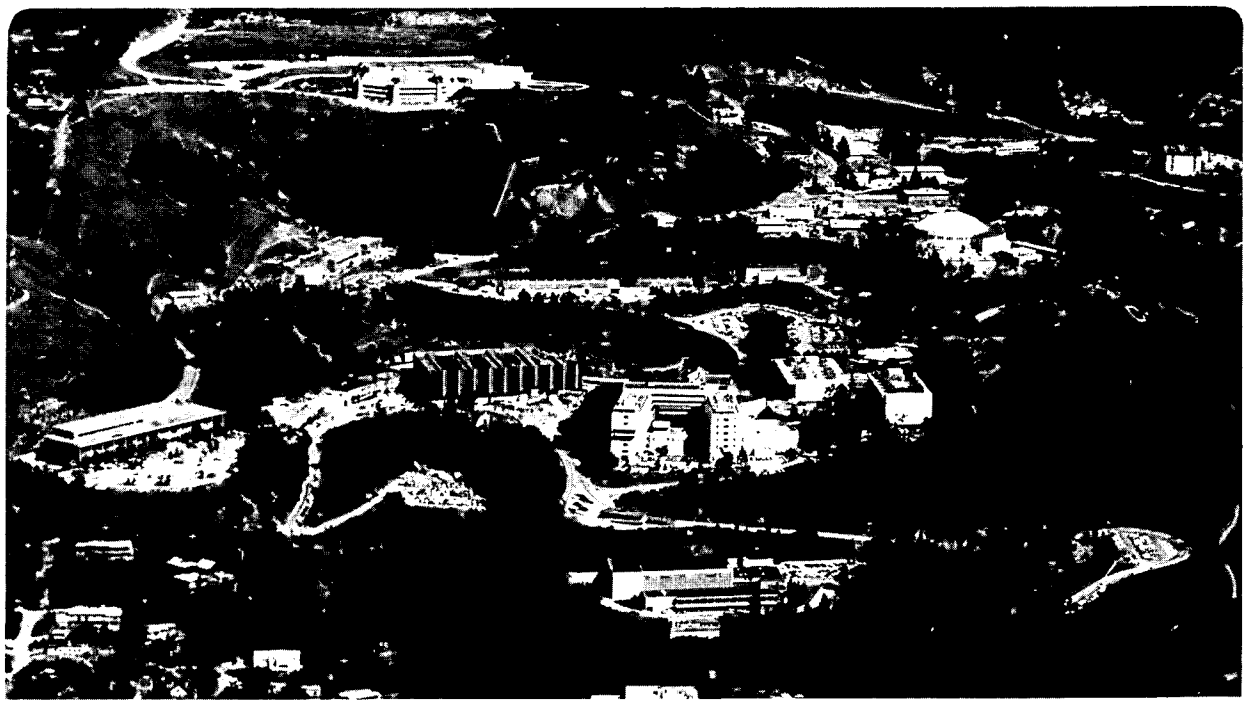

LBID-511
c.1

DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.

LAWRENCE BERKELEY LABORATORY - UNIVERSITY OF CALIFORNIA
ENGINEERING NOTE

MME Book No. 630B | FILE NO. MT 296 | PAGE 1 of 7

SUBJECT: Coil Calibration of 10 Coils - Test Results
Drawing No. 19M5696

NAME: Donald H. Nelson
DATE: June 15, 1981

Introduction

On May 20, 1981, Ed Cyr and I calibrated (i.e., determined the area of) 10 coils. Six of these coils are to be installed in a six coil array to be used for harmonic measurements of a superconducting magnet Isabelle prototype scheduled for measurements starting August 1, 1981. On May 22nd, we made more accurate determinations of the relative area of coils 2 through 10 (relative to coil 1 arbitrarily selected as the standard for comparison). On May 26th, we demonstrated the measurement technique to M.I. Green, W.V. Hassenzahl and T. Lauritzen.

Results

Table I summarizes the areas as determined by method 1, May 20th. See Test Plan - MT 295.

Table II shows the results of the comparative measurements (method 2 of MT 295) made on May 22nd and May 26th. For comparison I have included relative areas based on the absolute (but less accurate) measurements represented by Table I data in Table II.

Based on these data, we selected coil pairs and spares as shown in Table III. The choice of which coil of each pair would be selected as the outer coil was left to Lauritzen's discretion. Since the outer radius coils are most sensitive to errors in fabrication, we recommended that coils with loose turns be positioned to the inside position. Engineering drawing no. 19M5696 shows the coil locations in the array.

Method of Measurements

Method 1: We followed the procedures described in the test plan. For method 1, we measured magnetic induction over the 45 cm occupied by the coil centerline when in place. Measurements made both before and after the absolute calibration of the coil are represented by Figure 1. I numerically integrated these equally spaced data then

RL-398 7600-54257 (Rev. 9/73)

LAWRENCE BERKELEY LABORATORY - UNIVERSITY OF CALIFORNIA

ENGINEERING NOTE

MME Book No. 630B | FILE NO. MT 296 | PAGE 2 of 7

SUBJECT: Coil Calibration of 10 Coils - Test Results
Drawing No. 19M5696

NAME: Donald H. Nelson

DATE: June 15, 1981

Coil	Area (m^2)	Area (rpt.) (m^2)	Δ Area (%)	Dev from Average (m^2)	Dev from Average (%)	Dev of (rpt.) (m^2)	Dev of (rpt.) (%)
1	16.722			0.026	0.156		
2	16.682			-0.014	-0.084		
3	16.671	16.658	(-0.08%)	-0.025	-0.150	-0.038	-0.023
4	16.678			-0.018	-0.108		
5	16.705			0.009	0.054		
6	16.693			-0.003	-0.018		
7	16.677			-0.019	-0.114		
8	16.706	16.704	(-0.01%)	0.010	0.060	0.008	0.048
9	16.691			0.005	-0.030		
10	16.735	16.722	(-0.08%)	0.039	0.234	0.026	0.156
AVG	16.696						

TABLE I Coil Area Summary (Method 1)

LAWRENCE BERKELEY LABORATORY - UNIVERSITY OF CALIFORNIA

ENGINEERING NOTE

MME Book No. 630B | FILE NO. MT 296 | PAGE 3 of 7

SUBJECT: Coil Calibration of 10 Coils - Test Results
Drawing No. 19M5696

NAME: Donald H. Nelson

DATE: June 15, 1981

	HIGH PRECISION (RELATIVE AREAS)			ABSOLUTE AREA DATA DEVIATION* USING TABLE I DATA	
		REPEAT			
Coil No.	Deviation* (%)	No. 1 as Ref	No. 8 as Ref	Main Data (%)	Repeat Data (%)
2	-0.27			-0.24	
3	-0.35			-0.30	-0.38
4	-0.33		-0.29	-0.26	
5	-0.11			-0.10	
6	-0.20			-0.17	
7	-0.30			-0.27	
8	-0.11		(Ref)	-0.10	-0.11
9	-0.24	-0.21	-0.22	-0.19	
10	0.03			0.08	0.00

*Deviation with respect to coil no. 1

TABLE II Comparative Data With Comparisons to Absolute (Table I) Data

Coil Pair	Selected Coils		Spare
A	4	7	3
B	5	8	10
C	6	9	2

TABLE III Pair Selection

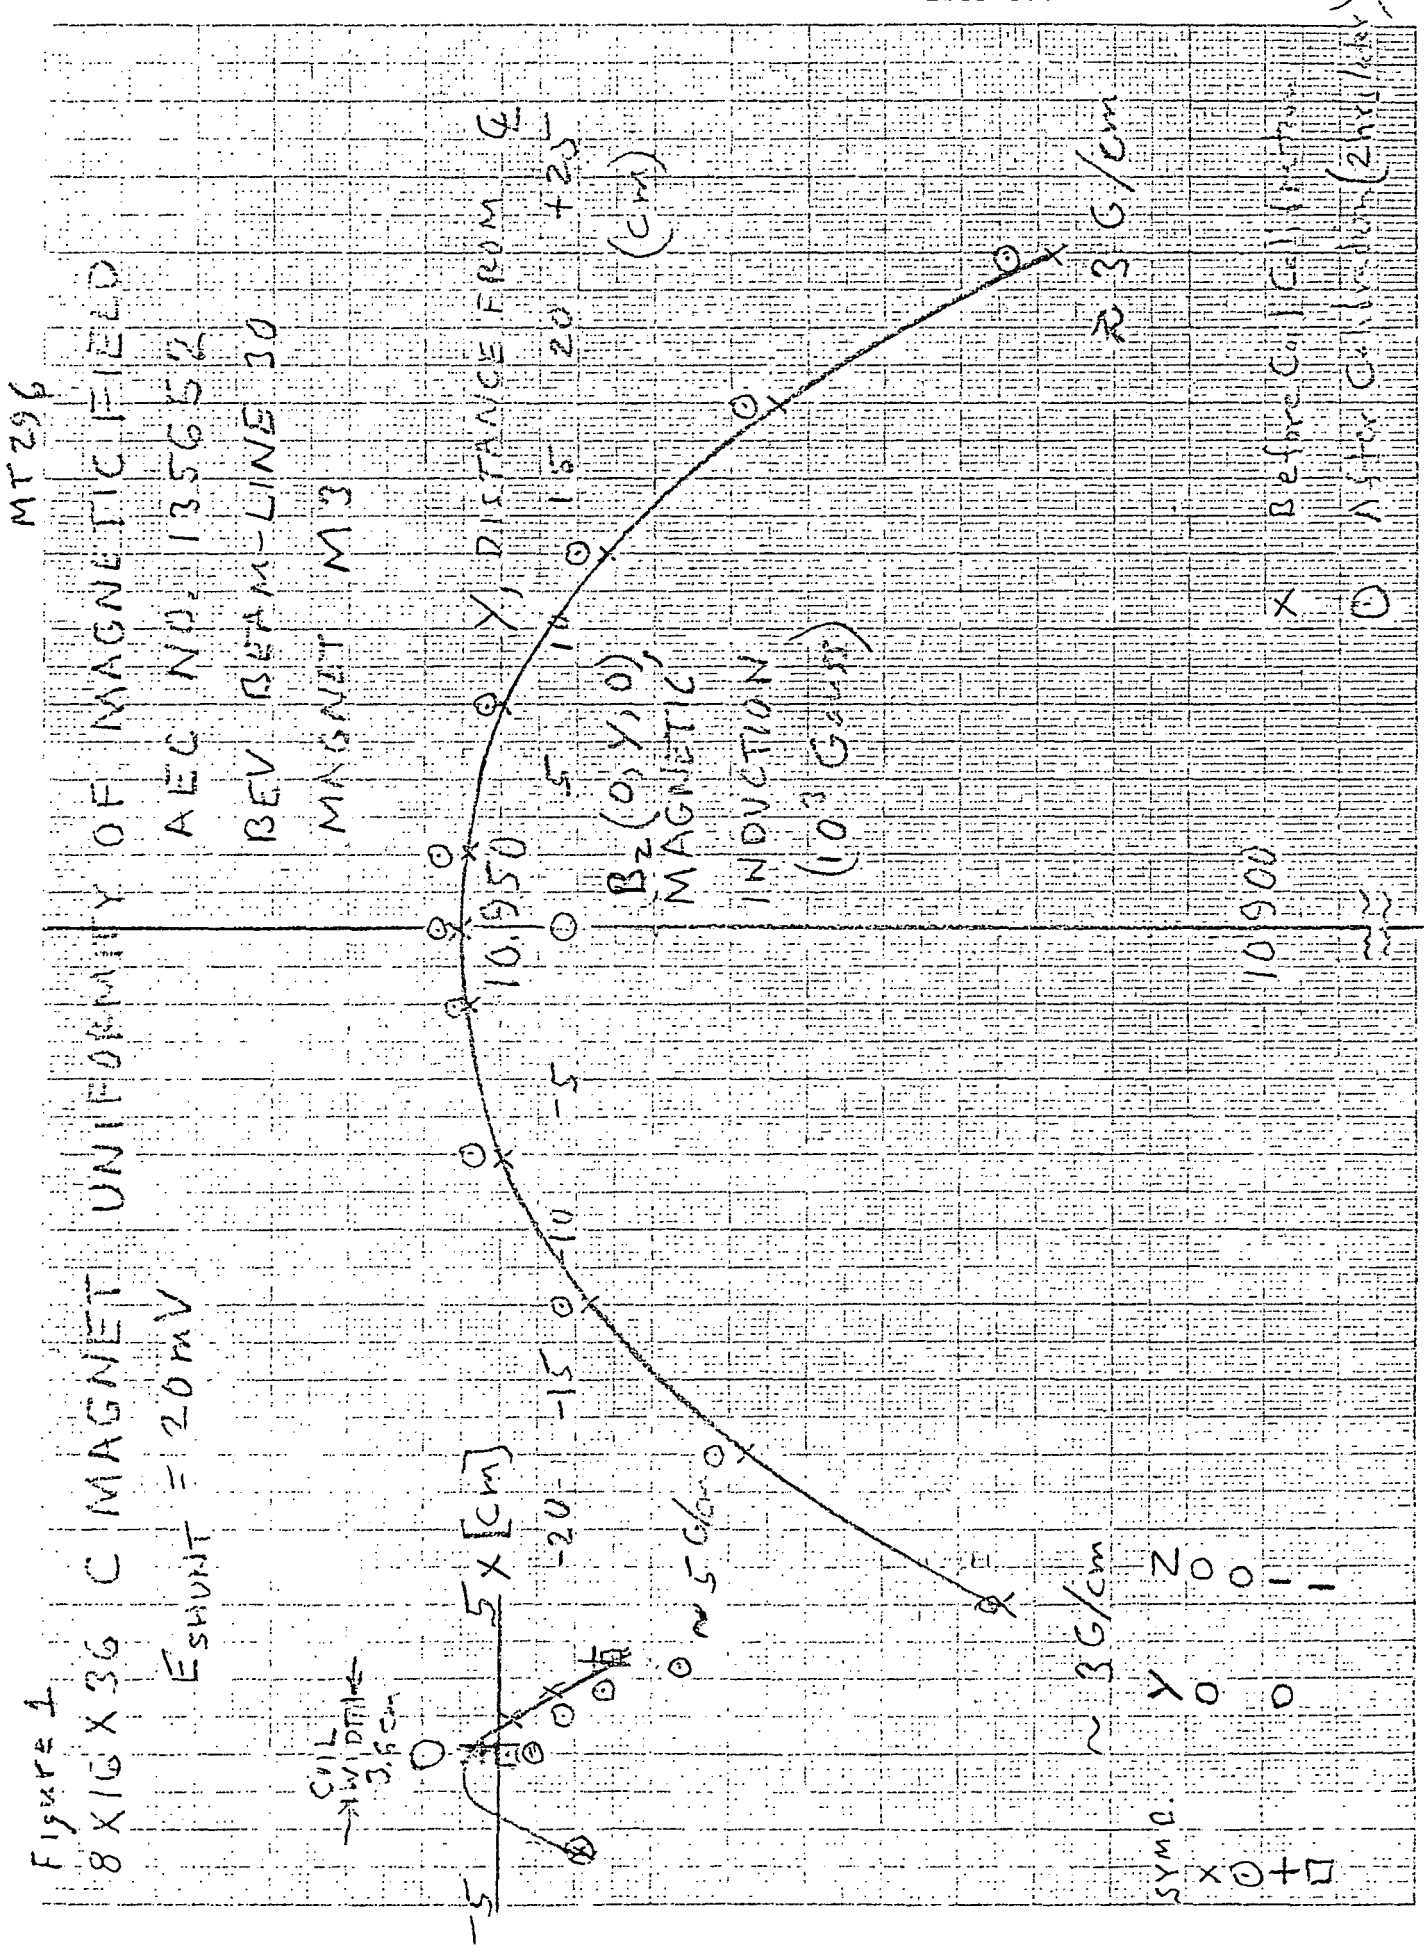
MT296
Figure 1
8 X 16 X 36 C MAGNET UNIFORMITY OF MAGNETIC FIELD
AEC NO. 135652
BEV BEAM-LINE 30
MAGNET M3
E SHUNT = 20 mV
Y, DISTANCE FROM ℄
(cm)
B2 (0, Y, 0), MAGNETIC INDUCTION (10^3 Gauss)
10,950
10,900
5 X [cm]
~ 5 G/cm
~ 3 G/cm
≈ 3 G/cm
COIL WIDTH 3.6 cm
SYMB.
Y
Z
Before Coil Calibration
After Calibration (2 hrs later)

divided by 45 cm to determine the average field over the coil volume. The HP 97 program used for performing the integration is saved in MME Data Book No. 630B. The before and after (calibration) determinations of average magnetic induction agreed to 0.02%.

We calibrated the electronic integrator with a flux standard and determined each coil area based on 1) a known flux linkage from the flux standard, and 2) a determination of B_{AVG} from the NMR data by solving equation 1.

$$nA = \frac{\psi_{SLFS}\ 1/2\ E_{Flip\ Coil}}{B_{AVG}\ E_{SLFS}} \qquad (1)$$

nA = turns area of coil under test (m^2)

ψ_{SLFS} = flux linkage provided by the SLFS (Wb)

B_{AVG} = average magnetic induction over the coil length (T)

$E_{Flip\ Coil}$ = output potential of integrator generated by flipping the coil in known magnetic induction (B_{AVG}) (V)

E_{SLFS} = output potential of integrator generated by a known calibration signal from the SLFS, i.e., due to ψ_{SLFS} (V)

Method 2: The second method described in the test plan is inherently a more accurate determination of coil area based on a known area reference coil. In selecting coil pairs, it is more important that the relative areas be known than the absolute, so we did not require knowledge of the area of the reference coil to high accuracy.

Method 2 is more accurate than method 1 because 1) there are fewer variables involved in the calibration, e.g., a knowledge of the magnitude of the field is unimportant, only that it doesn't change over the relatively short time of comparison, 2) only short term reproducibility of both the magnetic field and the measurement system gain are needed for method 2; whereas stability over the entire measurement period is required for method 1.

An HP 97 program using equations from the test plan (Method 2 - V-D) was used to determine the relative areas of the coils. This program is listed in MME Book No. 630B.

Discussion

Based on the few repeats, I estimate that the absolute calibration data is good to ±0.1% as predicted. The high precision data is probably ±0.02%.

The determination of areas by Method 1 was facilitated by the outstanding performance of the LBL/CERN Nuclear Magnetic Resonance Magnetometer. The success of these NMR systems is largely due to the effort of Dr. Michael I. Green

Distribution

W.S. Gilbert
M.I. Green
E.C. Hartwig/L.J. Wagner/W.H. Deuser
W.V. Hassenzahl
T. Lauritzen
R.M. Main
D.J. Rondeau
C.E. Taylor

This work was supported by the U.S. Dept. of Energy under Contract DE-AC03-76SF00098.

This report was done with support from the Department of Energy. Any conclusions or opinions expressed in this report represent solely those of the author(s) and not necessarily those of The Regents of the University of California, the Lawrence Berkeley Laboratory or the Department of Energy.

Reference to a company or product name does not imply approval or recommendation of the product by the University of California or the U.S. Department of Energy to the exclusion of others that may be suitable.

TECHNICAL INFORMATION DEPARTMENT
LAWRENCE BERKELEY LABORATORY
UNIVERSITY OF CALIFORNIA
BERKELEY, CALIFORNIA 94720